

Super Low Resolution RF Powered Accelerometers for Alerting on Hospitalized Patient Bed Exits

Michael Chesser*, Asangi Jayatilaka*, Renuka Visvanathan[†], Christophe Fumeaux[‡] Alanson Sample[§] and Damith C. Ranasinghe*

* Auto-ID Lab, School of Computer Science, The University of Adelaide, SA 5005 Australia
Email: {michael.chesser, asangi.jayatilaka, damith.ranasinghe}@adelaide.edu.au

[†]The Queen Elizabeth Hospital, Woodville SA 5011, Australia
Email: Renuka.Visvanathan@sa.gov.au

[‡] School of Electrical and Electronic Engineering, The University of Adelaide, SA 5005, Australia
Email: christophe.fumeaux@adelaide.edu.au

[§] School of Electrical Engineering and Computer Science, University of Michigan, MI 48109, USA
Email: aps@umich.edu

Abstract—Falls have serious consequences and are prevalent in acute hospitals and nursing homes caring for older people. Most falls occur in bedrooms and near the bed. Technological interventions to mitigate the risk of falling aim to automatically monitor bed-exit events and subsequently alert health care personnel to provide timely supervisions. We observe that frequency-domain information related to patient activity predominantly exist in very low frequencies. Therefore, we recognize the potential to use ultra low resolution acceleration information without the need to power a traditional MEMS (Micro Electro Mechanical System) based sensor. Consequently, we investigate a pervasive sensing modality with low cost batteryless or wirelessly powered Radio Frequency Identification (RFID) technology, with the potential for convenient integration into *clothing*, such as hospital gowns. We design and build an ultra low resolution passive accelerometer-based RFID sensor embodiment (*ID-Sensor* approach) for our study. The sensor design allows deriving ultra low resolution accelerometric data from the rate of change of unique RFID tag identifiers in accordance with the movement of a patient's upper body. We investigate dense labelling of patient activity sequences from the RFID data stream using a fully convolutional network (FCN) and compare this network architecture with a state-of-the-art network for human activity recognition as well as a traditional machine learning method with engineered features. We demonstrate that the low resolution RF powered acceleration data embedded in the data stream provides a practicable method for patient bed-exit detection where features can be efficiently learned using a FCN architecture. We evaluate performance, true alarms and false alarms, with 25 hospitalized older patients.

I. INTRODUCTION

The world population is rapidly ageing and in the year 2050 approximately 2 billion people will be 60 years of age or older [1]. Therefore ageing associated issues such as increased risk of falling are becoming prevalent. Approximately 30-50% of older people living in long-term care institutions fall each year [2]. Falls in residential care or hospitals lead to many adverse consequences on the patients apart from physical injuries such as anxiety, depression and loss of independence [3], [4]. Furthermore, falls are costly because they increase the length of hospital stays. A recent study estimated the total medical costs for falls in 2015 at approximately \$50 billion USD in the United States alone [5]. In residential care and hospitals, falls

commonly occur near and around the patients' beds [3]. A recent study, a first of its kind, conducted an in-depth analysis of video surveillance recordings over three years and revealed that people fall as a result of getting out of bed and also as a result of walking [4].

Automatically recognizing patients leaving their bed in real time provides an opportunity to intervene and supervise unattended patients. A common strategy to provide targeted care to older patients in hospitals is by using automatic alarm systems. Alarm systems issue a warning when a patient is getting out of bed with the aim of staff promptly attending to the patient and thereby potentially reducing the risk of a fall or rendering immediate assistance in case of a fall [6]–[8]. Such systems, focused on prevention are more desirable than systems focused on detecting a fall after the event has *already* occurred [8]. Current approaches to recognize bed-exits using pressure sensors—for example pressure mats [9], [10]—are shown to be ineffective in reducing falls in clinical trials [11]. Older people have expressed privacy concerns with the use of camera based technologies [12]. Recent studies have explored battery-powered body worn sensors for patient activity recognition [8], [13]; however, these sensors are expensive¹, require manual attachments, maintenance and battery replacements, and strapping to the body as in [13].

In contrast, we postulate an alternative. We observe that patient activity related information in the frequency-domain is found in very low frequencies of typically less than 4 Hz [14]. Therefore, we recognize the potential to use ultra low resolution acceleration information without the need to power a traditional MEMS (Micro-Electro-Mechanical Systems) based sensor to gather human motion information. Consequently, we design an RF (radio frequency) powered or passive sensing modality with low cost batteryless Radio Frequency Identification (RFID) technology with the potential for convenient integration into *clothing*, such as hospital gowns. In particular,

¹MbientLab Bluetooth sensor pricing (these prices do not include the cost of coin cell batteries) <https://mbientlab.com/pricing/>

we investigate the efficacy of embedded acceleration data extracted from the modulation of two unique identifiers in an RFID data stream. The change in identifiers or IDs in accordance with human motion data is derived from a tag with two commercial off-the-shelf (COTS) RFID circuit modules as illustrated in Figure 1b.

There are many advantages to using passive wearable UHF RFID for capturing the movements of older patients: *i*) passive devices have potential for an indefinite operational life without requiring maintenance or battery replacements; *ii*) wearable RFID technology addresses the problem of distinguishing individual patients from multiple others, faced by most device-free sensing schemes and allows individualizing bed-exit alarms to match patient needs over time; and *iii*) RFID tags are low-cost (7-15 U.S. cents) [15], hence, disposable to support infection control protocols in hospitals. Furthermore machine washable RFID tags are now commercially available and can be easily woven into hospital garments [16] creating possibilities for unobtrusive monitoring of patient activities. Unobtrusiveness has been identified as a key acceptance criteria by older people [17], [18]; a necessary condition for translating technology into practice. Most notably, we see an increasing technology trend to integrate RFID technology with textiles [19].

We have seen demonstrated capability to use commercially available passive UHF RFID technology for recognizing human interactions with RFID tagged objects [20]–[22], tracking of objects or people [23], [24], as well as use of large number of body-attached RFID tags for human motion tracking [25], [26]. However, our study is a *first-of-its-kind*. To the best of our knowledge: *i*) the potential to extract and use low resolution acceleration data from an extremely low power method for human activity recognition; and *ii*) a practicable means for recognizing bed egress motion for a clinical application with a worn RFID tag and the evaluation with a target demographic of frail older hospitalized people have not been previously investigated.

A. Contributions

Our main contributions of this paper are given below.

- We investigate a new and pragmatic human motion sensing approach. We observe that patient activity related information in the frequency-domain exist in very low frequencies. We construct a prototype RFID device—*ID-Sensor*—using only low cost commercially available RFID Integrated Circuits (ICs) to obtain ultra low resolution acceleration data. We show that the *ID-Sensor* provides a unique ability to capturing human motion information without a conventional accelerometer.
- We consider a fully convolutional neural network (FCN) architecture capable of dense labelling and predictions. This is a natural formulation as human activity recognition is essentially a sequence labelling problem where a class label is estimated for each sensor sample in a time series. We demonstrate that effective features can be learned from our unique *ID-Sensor* data stream by

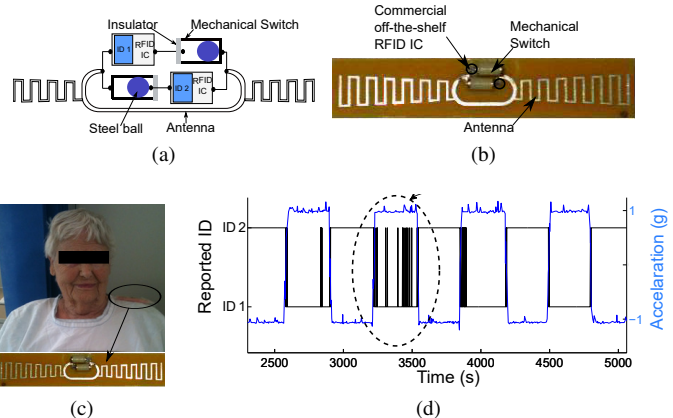


Fig. 1. (a) Design of the RFID sensor tag. Each RFID Integrated Circuit (IC) has a unique tag ID. As a result of only one RFID IC being attached to the antenna, only one ID will be reported by the RFID platform at a given time. This figure illustrates the state of the *ID-Sensor* when ID 2 is reported. (b) *ID-Sensor*: The batteryless RFID sensor tag prototype used in our experiments. (c) A patient wearing the batteryless RFID tag attached at the shoulder level to a hospital garment. (d) Comparison of the ID reported by the *ID-Sensor* against acceleration values obtained from a MEMS accelerometer.

comparing performance with engineered features and a traditional machine learning method.

- We conduct a pilot study with 25 hospitalized older patients. We demonstrate the efficacy of our approach for recognizing bed exits with learned features and classifier from the FCN. In particular, our experimental study is conducted in a realistic experimental setting and with a demographic of participants intended for the application. We demonstrate the capability to employ a single low cost body-worn passive UHF RFID tag for sensing of patient activities.
- We release a new activity dataset collected from hospitalized older people to the research community—available from [27].

We defer related work to Section VII. In the following sections we describe our sensor construction and operation, followed by the experimental design and the machine learning approaches we formulate for the activity recognition task. We discuss our results and conclude our paper in Section VIII.

II. PASSIVE RFID-BASED ID-SENSOR

Passive RFID tags harvest energy radiated by an RFID reader antenna and once successfully powered, responds by backscattering the Radio Frequency (RF) signals back to the RFID reader antenna. Apart from the unique electronic identifier sent from a tag, modern RFID readers are able to measure detailed RF communication-related properties such as received signal strength expressed as RSSI and phase difference of the received signal. While information extracted from RSSI has been exploited in the past, the exploitation of information related to *changes in phase* information are rarely explored for human activity recognition. We aim to exploit both of these information sources. Notably, both phase and RSSI related information is extracted at no additional

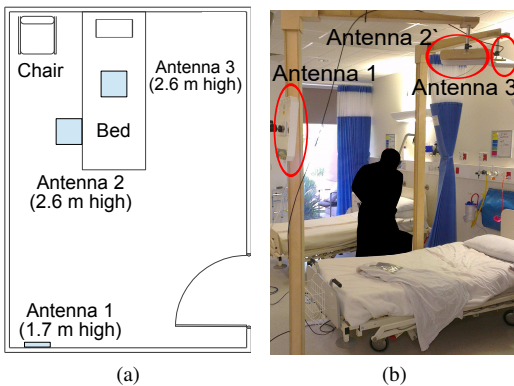


Fig. 2. (a) Typical layout of a hospital bed room. The picture shows a single bed room used in our experimental study and indicates the reader antenna locations. (b) Experimental set up in a double bed room.

computational or power burden to the tag and thus does not impact the reading range or the performance of the tag.

Our goal is to create and exploit another such information source for human activity recognition.

We employ low-cost batteryless RFID technology to build our *ID-Sensor* to capture low frequency information related to human motion. We developed this prototype based on [28]. The platform consists of two antiparallel mechanical tilt switches and two RFID Integrated Circuits (ICs) attached to a single Radio Frequency (RF) antenna on a Printed Circuit Board (PCB) substrate (see Fig. 1a and Fig. 1b). Since the mechanical switches are attached opposite to each other, only one RFID IC is attached to the antenna at a time. Each RFID IC has a unique tag ID (ID1 or ID2). Starting from the case where the first RFID IC is connected, flipping (or shaking) the tag will result in the first IC becoming disconnected, and the second RFID IC becoming connected to the antenna. At a given time, the ID stored in the RFID IC connected to the antenna will be reported by the platform. Thus, tilt and accelerometer data are encoded as *modulations* between the two IDs reported back to the reader.

The key concept here is the exploitation of two tiny batteryless UHF RFID tag ICs in a configuration that allows switching between the ICs based on the direction of the gravitational force vector in relation to a human body reference frame. Most notably, the accelerometer in essence consumes no electrical power, or more accurately, is limited to the negligible Ohmic losses of the switching element. Importantly, the *ID-Sensor* uses low-cost readily available components, is mass producible, and has RF performance equivalent to conventional single IC RFID tags. Furthermore, patients are precisely and automatically identified by the unique electronic identifiers stored in the worn RFID tags.

Figure 1d compares the low resolution acceleration information received from the *ID-Sensor* with acceleration values obtained using a MEMS accelerometer (ADXL330). This was obtained by rotating both *ID-Sensor* and the accelerometer at an identical rotational velocity. We can see that the ID reported

by the *ID-Sensor* is capable of representing the direction of the gravitational force vector and rate of rotation or angular acceleration. However, it is also evident that the ID reported by the *ID-Sensor* can sometimes result in noisy measurements as highlighted in Fig. 1d. This is due to the steel ball failing to disconnect at times and as a result connecting both RFID ICs to the antenna simultaneously.

Therefore, our study will investigate the ability to use this noisy low resolution acceleration information for human activity recognition problems.

The consideration of whether the noisy acceleration data provides any additional information forms the basis for the two approaches we will investigate:

- **ID-Sensor Approach:** Here, we utilize the embedded acceleration data in the form of changes in IDs from our *ID-Sensor* in addition to RSSI and phase information.
- **Tag Approach:** We ignore the ID modulation information and we treat *ID-Sensor* as a simple commercial off-the-shelf (COTS) batteryless UHF RFID tag. Hence we do not distinguish between ID1 and ID2 and instead treat them as a single identifier.

III. EXPERIMENTAL STUDY

The participants for our experimental study were inpatients at the Geriatric Evaluation and Management Unit of the Queen Elizabeth Hospital, South Australia. The patients selected for the study were able to consent to the study and mobilize independently. This study had ethics approval from the human research ethics committee of the Queen Elizabeth Hospital, South Australia (2011129). We describe the details of the data collection and experimental settings below.

Participants: Twenty five older participants were recruited (age: 84.4 ± 5.3 years, height: 1.68 ± 0.09 m) for the study with the help of geriatricians. All participants provided informed consent and no honorarium was paid. The study was completed over a six-month period where each trial with each volunteer lasted between 60 to 90 minutes. The *ID-Sensor* was attached to the loosely fitted hospital gown and over a participant's shoulder as shown in Fig. 1c.

Settings: The data collection occurred in the individual rooms of patients consenting to the study. These patient rooms included both double and single bed rooms. The furniture and, hence, the antenna deployment in all the patient rooms were similar. The generic deployment of antennas used in the experiments is illustrated in Fig. 2a and Fig. 2b. During trials the position of the back rest on a bed was not fixed and was generally elevated slightly to suit the personal comfort of individual patients. Although the room setting was mostly fixed during the experiment, movement of other people (such as nurses) was not restricted.

We used an Impinj Speedway Revolution reader operating at the regulated Australian RF frequency band of 920-926 MHz and a maximum regulated power of 1 W. The communication between the RFID tag and the reader is governed by the ISO-18000-6C air interface protocol. In this study, three antennas

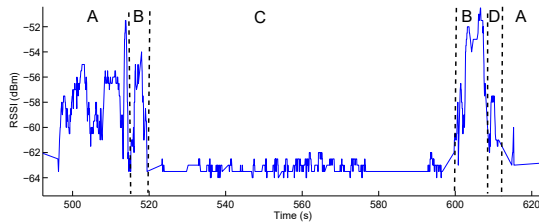


Fig. 3. Typical variations in RSSI values for *in-bed* and *out-of-bed* activities. Here, A: walking, B: Sitting on bed, C: lying on bed and D: Standing

were attached to the RFID reader and strategically deployed in patient's rooms (see Fig. 2a and Fig. 2b). The antenna deployment was designed to illuminate the area covering the bed and chair. The read distance of UHF RFID tags in free space is generally 10m. In the experimental set-up, the read rate (or sampling rate) of the *ID-Sensor* was approximately 20 reads per second.

Data collection: Since our study participants were hospitalized older frail patients, it was observed that most of their time was spent lying in bed. Therefore, in order obtain sufficient amount of information for bed-exit events, and to minimize the physical and mental stress for the participants, the study was conducted using broadly scripted activity routines to allow us to obtain an adequate number of bed exit events.

The participants were instructed, prior to each trial, to lie on the bed in a manner most natural and comfortable to them. They were requested to get out of the bed during the experiment and no specific instructions were given about how or when to get out of the bed. As they were frail patients, the number of times each patient got out of the bed was not fixed and was dependent on their physical abilities. They were allowed to perform other activities while *in-bed* as well as while *out-of-bed*. Typical *in-bed* activities involved lying, sitting, watching a television, drinking and reading. Typical *out-of-bed* activities involved standing and walking. Given the very limited number of activities a patient can perform in a hospitalized environment, we believe these activities represent adequate class diversity. Given the varying physical abilities of our patient group, we also benefited from very high intra-class diversity. A researcher annotated the activities being undertaken. Given our interest in bed egress motions, two ground truth activity labels were considered for our study: i) *in-bed*; and ii) *out-of-bed*.

Data set: The total data set contains 244,440 tag readings which included 107,439 *in-bed* and 137,001 *out-of-bed* related tag readings. Read rate (or sampling rate) was generally between 5-20 reads per second. The data set included 77 bed-exit events (i.e. transitions from *in-bed* to *out-of-bed*).

IV. APPROACH

A bed-exit event is recognized as a transition from *in-bed* to *out-of-bed*. Once a bed-exit is identified, interested parties, such as caregivers, can be notified, by means of a pager message or phone notification as discussed in [8],

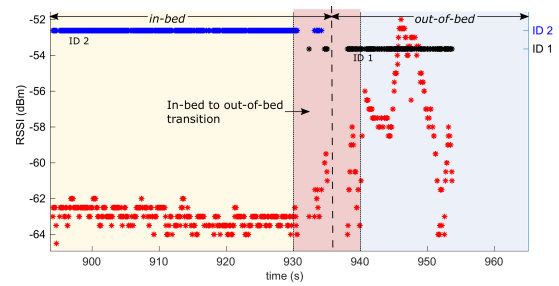


Fig. 4. Capture of a bed-exit posture transition of a patient where the ground truth changes from *in-bed* to *out-of-bed*. Changes in ID information embed low resolution accelerations using the *ID-Sensor*. We can also observe typical RSSI patterns associated with the activated ID of the *ID-Sensor* prior to, during and after the activity transition.

[18]. Our approach to recognize bed-exits is built around the observations that: i) human motion information can be extracted from the channel state measurements, RSSI and phase, made by an RFID reader; and ii) low frequency information associated with patient movements from the *ID-Sensor* where the data stream from the reader can be also be used to extract low resolution acceleration information. Importantly, we can extract all three information sources without a power burden on the tag and through standard interrogation of the *ID-Sensor*. However, all of these measurements are noisy; the challenge is to learn the hidden patterns to recognize bed egress motions from noisy data. We discuss these information sources briefly.

Signal strength information: RSSI is an indicator of the power of the tag signal received by an RFID reader antenna [29]. RSSI is predominantly affected by the distance between the reader and the tag as well as the orientation of the tag antenna. Based on the Friis transmission equation, RSSI of a backscattered signal that is captured by an RFID reader has the form of $P_t G_t^2 G_{path}^2 K$. Here, P_t is the output power of the reader, G_t is the gain of the reader antenna, K is the backscatter gain. The G_{path} is the one-way path gain of the deterministic multipath channel determined as $G_{path} = \left(\frac{\lambda}{4\pi R}\right)^2 |H|$. Here, R is the line of sight distance between the tag and the reader antenna, and H is the channel response due to multipath and channel absorption characteristics. For instance $H \propto e^{-\alpha R}$ where α is the absorption coefficient of the medium. We can see that although RSSI is sensitive to channel characteristics, it is predominately determined by R as $RSSI \propto 1/R^4$.

Figure 3 illustrates data collected using reader antenna 3 for a sequence of activities related to getting into bed and then getting out of bed. From Fig. 3 we can observe that RSSI is sensitive to movements. For instance, the posture transition from *lying on bed* to *sitting on bed* (i.e. in Fig. 3, from C to B) has resulted in a notable increase in RSSI value while the posture transition from *sitting on bed* to *standing* (i.e. in Fig. 3, from B to D during 600s to 620s) has resulted in a decrease in the RSSI value.

ID-Sensor information: We have illustrated in Fig. 1d and

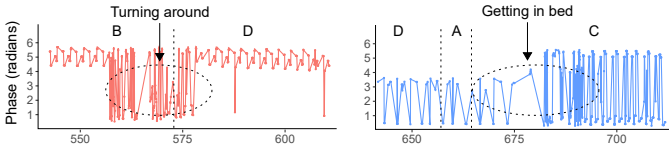


Fig. 5. An extract of variations in instantaneous phase values for *in-bed* and *out-of-bed* activities of two antennas (red: antenna 1, blue: antenna 3). Where A: walking, B: Sitting on bed, C: lying on bed and D: Standing

discussed in Section II the capability of obtaining acceleration data by considering the ID modulations within the RFID data stream. As observed in Fig. 4, changes in the reported IDs are likely to be observed for a patient's upper body movement such as during a bed egress activity. This is a consequence of the sensor moving in accordance with a patient's upper body movements and rotations that changes the orientation of the sensor's mechanical switches with respect to the gravitational force vector resulting in modulations between ID1 and ID2 of the sensor. These modulations capture low frequency acceleration information associated with human motions. Further, we observe that RSSI patterns captured by each activated ID generally differ according to a patient's lying and standing posture as well as during a posture transition (see Fig. 4). Therefore, RSSI patterns specific to each ID provide further movement information.

Phase information: Phase estimates from an RFID reader is a measure of the phase angle between the RF carrier transmitted by the reader and the return signal from the tag. RFID readers performs frequency hopping from one channel to another. As a result, phase values are dependent on the carrier frequency. Phase estimates are related to two motion information sources: *i*, for a given frequency, the phase of the tag signal at two different time instances can estimate the tag's radial velocity as $V_r \propto \frac{\partial \Psi}{\partial t}$; and *ii*) the distance between an RFID reader antenna and the RFID tag is proportional to the partial derivative of the phase with respect to the derivative of channel frequency as $d \propto \frac{\partial \Psi}{\partial f}$. Given the sensitivity of phase information to small changes in distance, we can expect phase data to capture activity transition information. Figure 5 shows an extract of variations in phase information across two activity transitions in our dataset. We can observe that RF phase (Ψ) is generally affected by even small movements of an RFID tag while RSSI is primarily affected by much larger movements.

A. Classification Problem

We are interested in determining the associated activity label (*in-bed* or *out-of-bed*) for each *ID-Sensor* reading. We treat the problem of determining whether a patient is *in-bed* or *out-of-bed* to be a binary classification problem. Subsequently, a bed-exit event is recognized as a change in classification from *in-bed* to *out-of-bed*.

The data sequence collected is a time series and a single tag reading consists of the 4-tuple: i) reader antenna ID (aID); ii) RSSI; iii) Phase; and iv) tag ID (ID). It is important to transform the received data sequence into a suitable representation

before applying activity-based machine-learning models. The most common strategy is to segment the time series. We used a fixed time sliding window, however, the selection of segment size (δs) is an empirical process determined by each algorithm. Our goal is to investigate a classical machine learning method with a feature learning method based on state-of-the-art neural network architectures used with kinematic sensor data. We recognize that the nature of RFID data is significantly different from kinematic sensor data and feature learning from RFID data streams for activity recognition remains to be explored. Therefore, we use the classical machine learning method of Logistic Regression (LR) with engineered features as a benchmark to compare with two deep neural network architectures.

B. Logistic Regression

In this study, we used a classical machine learning algorithm capable of generating probabilistic models using feature vectors extracted from segments. LR assumes that the training data, (x_t, y_t) where $t \in \mathbb{N}$, $x_t \in \mathbb{R}^d$ is the feature vector and $y_t \in \{-1, +1\}$, is the class label, are independent and identically distributed. LR models the conditional probability $Pr(y_t = 1|x_t)$ as follows:

$$Pr(y_t = 1|x_t) = \left(\frac{e^{\langle w, x_t \rangle}}{1 + e^{\langle w, x_t \rangle}} \right) = \left(\frac{1}{1 + e^{-\langle w, x_t \rangle}} \right)$$

here w is the learned model.

We engineered a number of features using the information available in a given segment with respect to: *i*) RSSI; and *ii*) correlation between participant's movements and antennas capturing tag readings. Additional features utilizing one-bit acceleration were engineered for the *ID-Sensor* approach (see Table I).

Features based on RSSI: For a given segment S_i with respect to a given tag reading, i , we used the features summarized in Table I and also used in [18], [30]. In order to further capture the changes in RSSI for short distance movements, we introduce new a binary feature $M \in [0, 1]^{|A|}$ to determine whether a patient is moving towards or away from a fixed antenna within S_i where M_k is defined as:

$$M_k = \mathbf{1}_{[t_{\max(S_i(RSSI^k))} > t_{\min(S_i(RSSI^k))}]}, \quad (1)$$

where $k \in \mathcal{A}$ and $\mathbf{1}_x$ assumes 1 if x is true and 0 otherwise. \mathcal{A} is the set of antennas in the deployment. Although the proposed binary feature M_k can be used to identify human movements within a segment, it cannot be used to recognize trends in the RSSI values over a longer period. To capture these patterns we considered a longer segment \mathfrak{S}_i of size $3\delta s$ with three equal sub-segments $\mathfrak{S}_i^j, j = 1, \dots, 3$. We consider the mean value of RSSI in each sub-segment. Since $\mathfrak{S}_i^3 = S_i$ we only include mean RSSI value for $\mathfrak{S}_i^j, j = 1, 2$.

Features based on correlation between participant's movements and antennas capturing the tag readings: It was observed that the antennas that collect readings differ depending on the location and movements of the patient. The RFID antenna facing the RFID tag are most likely to both power and collect data from the tag.

TABLE I
FEATURES EXTRACTED FROM A SEGMENT

Notation	Description
RSSI based Features	
$RSSI_i$	Most recent RSSI value
$\text{mean}(S_i(RSSI^k))$	Mean RSSI value
$\text{max}(S_i(RSSI^k))$	Maximum value of the RSSI
$\text{min}(S_i(RSSI^k))$	Minimum value of the RSSI
$\text{std}(S_i(RSSI^k))$	Standard deviation of the RSSI
M_k	Whether the maximum RSSI value is followed by the minimum RSSI value
Phase based Features	
Ψ_i	Most recent phase value
$\text{median}(S_i(CFPR^k))$	Median of the CFPR
$\text{sum}(S_i(CFPR^k))$	Sum of the absolute values of the CFPR
$\text{std}(S_i(CFPR^k))$	Standard deviation of the CFPR
Event based Features	
RC_k	Relative read event count per antenna
ω_k	Antenna which corresponds to the majority of events in S_i
aID_i	The antenna ID corresponding to the most recent tag reading
Features Specific to ID-Sensor approach	
a_i	ID of the most recent tag reading
$ S_i(a=x) / S_i , x=1,2$	Relative ID count

* $k = 1, 2, 3$ (antenna number), i is number of the respective tag reading

First, we considered a feature that indicates the relative count of read events for each antenna ($RC \in \mathbb{R}^{|\mathcal{A}|}$) within S_i which is calculated as:

$$RC_k = \frac{|S_i(aID = k)|}{|S_i|}, \quad (2)$$

where $k \in \mathcal{A}$. Second, we introduced a vectorized binary feature, $\omega \in \{0, 1\}^{|\mathcal{A}|}$, to identify the antenna which corresponds to the majority of events in S_i , which takes values as:

$$\omega_k = \begin{cases} 1 & \text{if } k = \arg \max_{l \in \mathcal{A}} RC_l \\ 0 & \text{otherwise} \end{cases} \quad (3)$$

where ω_k represents the k^{th} position of the vector ω which corresponds to the antenna k .

Phase-based Features: In our study we used statistical features derived from phase measurements from each antenna as in [21], [22]. These features are summarized in Table I.

Specific Features Engineered for the ID-Sensor approach: We build the following features to extract the acceleration information available in a segment. The ID of the most recent tag reading (a_i) was considered as a feature as it approximates to a one-bit acceleration value. We included the relative ID count ($RI \in \mathbb{R}^2$), as a feature as it provides information about the changes in the IDs or rate of change information—see Figure 4—during the considered segment S_i . In order to allow the classifiers to learn from RSSI patterns specific to each ID as shown in Fig. 4, we extracted RSSI features described previously with respect to each reported ID. In total we extracted 15 features for the *Tag* approach and 17 features for *ID-Sensor* approach.

C. Neural Network approaches

Instead of engineering features, current research suggests that we can learn features from kinematic sensors and build a classifier using deep neural networks using raw readings.

We consider two state-of-the-art architectures: i) Deep Convolutional and LSTM Recurrent Neural Network; and ii) Fully Convolutional Neural Network architecture.

Deep Convolutional and LSTM Recurrent Neural Network (ConvLSTM): We design a network architecture following [31]. This network architecture has reported state-of-the-art performance on benchmark human activity datasets based on kinematic sensors. The convolutional layers learn to extract features under the independent and identically distributed assumption of the input segments while LSTM layers captures temporal dependencies in sequential data, such as the RFID data stream in our work. The network architecture we developed and used is described in Fig. 6a. Using the notation from [32] the network can be summarized as: $C(32)-C(16)-C(8)-C(2)-R(200)-R(200)$.

Fully Convolutional Neural Network (FCN): We design a fully-convolution-network (FCN) following the design in [24]. This network architecture is more convenient to train than LSTM based networks since it lacks any recurrent connections. In addition, the network fully convolutional architecture has reported new state-of-the-art performance measures for benchmark human activity recognition datasets with body worn kinematic sensors. Further, the FCN architecture addresses issues with window label ambiguity—the multi-class window problem [24] where windows overlap multiple classes while ground truth labels are limited to selecting, for example, the majority class as the ground truth label for a given segment. The network architecture we designed for our classification problem based on [24] is described in Fig. 6b. Using the notation from [32] the network can be summarized as: $C(10)-P-C(10)-P-C(10)-P-C(10)-P-C(10)-C(2)-S$.

As input, we use a minibatch size of 100, feeding the inputs [tag ID (a), aID , $RSSI$, and phase (Ψ)] as individual channels to the network. We use a window size of 30 for the ConvLSTM network and a window size of 64 for the FCN. For the ConvLSTM based network, we unroll the network 40 steps. Both networks were trained using gradient descent with the Adam optimizer until convergence. The code and model parameters for the networks used will be available at [27].

V. STATISTICAL ANALYSIS

Our main objective is to reduce the missed and false bed-exit events. Therefore, we selected precision (P) and recall (R) for our evaluation and measure performance using the F_1 -score (F) calculated as: $F = (2 \times P \times R)/(P + R)$.

In order to evaluate bed-exit event recognition performance we defined a true positive (TP) bed-exit event as: i) a bed-exit event that occurs no more than δt time before the actual bed-exit; or ii) a bed-exit event that is recognized while the patient is actually *out-of-bed*. False positive (FP) bed-exit events are incorrectly recognized bed-exit events based on the above definition of TP. Now, $P = TP/(TP + FP)$ and $R = TP/(TP + FN)$.

As our study participants were hospitalized older patients, we observed during our trials that while sitting on bed, often,

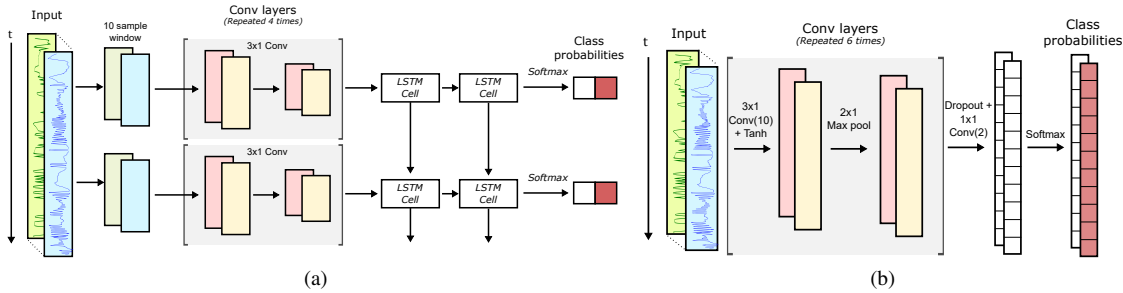


Fig. 6. a) An overview of the ConvLSTM network used. A 30 sample window is fed into a network consisting of 4 convolutional layers (4x1 convolutions with a stride of 2, tanh activation), followed by a dense RNN network (LSTM cells). Dropout (with a keep probability of 0.7) is applied to the inputs and outputs of each LSTM layer. We used strided convolutions and gradually reduce the number of features in the convolutional layers to achieve dimensionality reductions. This differs from the original network described in [31]. We found these choices performed better with the low information content of the raw sensor data. b) An overview of the FCN network used. We used 4 Conv/Max pool layers. Similar to [24] we kept the stride of Conv and Max-pool layers as 1. However, instead of using 2D convolutions we used 1D convolutions (3x1 kernels with tanh activation) which we found performed better with our data.

TABLE II
BED-EXIT PERFORMANCE WITH LEAVE ONE OUT CROSS VALIDATION

	F-Score	Recall	Precision
<i>Tag approach</i>			
LR	0.61	1.00	0.44
FCN	0.61	1.00	0.44
ConvLSTM	0.69	0.90	0.57
<i>ID-Sensor approach</i>			
LR	0.84	0.90	0.80
FCN	0.85	0.86	0.86
ConvLSTM	0.78	0.92	0.68

TABLE III
BED-EXIT RECOGNITION PERFORMANCE FOR EACH PATIENT USING FCN

Patient ID	Actual	<i>ID-Sensor</i>			<i>Tag</i>		
		TP	FN	FP	TP	FN	FP
0	2	2	0	0	2	0	0
1	3	3	0	0	3	0	1
2	2	2	0	0	2	0	7
3	3	3	0	0	3	0	6
4	3	1	2	0	3	0	3
5	3	3	0	0	3	0	5
6	2	2	0	1	2	0	8
7	3	3	0	0	3	0	1
8	1	1	0	0	1	0	2
9	6	3	3	0	6	0	0
10	3	3	0	0	3	0	2
11	3	2	1	0	3	0	6
12	3	3	0	1	3	0	7
13	2	2	0	0	2	0	12
14	3	3	0	1	3	0	1
15	3	3	0	0	3	0	4
16	3	3	0	0	3	0	2
17	7	4	3	0	7	0	4
18	3	3	0	3	3	0	3
19	3	3	0	0	3	0	1
20	3	2	1	2	3	0	1
21	3	3	0	1	3	0	7
22	3	3	0	0	3	0	0
23	3	3	0	0	3	0	7
24	4	3	1	2	4	0	8
Total	77	66	11	11	77	0	98

several attempts were required by patients to actually transition out of bed. Therefore, we analysed the sitting on bed durations (D) for patients before getting out of the bed and selected $\delta t = \text{mean}(D) + \text{std}(D) \approx 30$ s. In the study, bed-exit alarms are recognized as TPs as long as the patient is *out-of-bed* because people could fall during and after bed-exits [4]; hence, knowing that the patient has left the bed will provide the opportunity for the nurses to intervene and possibly prevent a fall or provide immediate assistance in case of a fall.

We evaluate our performance measures using *leave one patient out* cross validation. This validation approach is a participant independent testing scheme. This allows us to evaluate performance against a participant never seen during training or validation. Although this approach can show poor performance results, we can expect the results to be closer to that realized in a real world deployment.

VI. RESULTS

Table II illustrates performance obtained for bed-exit event recognition using leave one patient out cross validation. According to the mean F-Score, *ID-Sensor* approach has outperformed *Tag* approach. We can expect the higher performance of the *ID-Sensor* approach as a consequence of the information from the low resolution acceleration data embedded in ID modulations of the *ID-Sensor* approach (see Fig. 4).

We further analyzed the bed-exit event recognition performance in terms of TPs and FPs for each patient. The results are shown in Table III for the best performing method, FCN. We can see a significant reduction in FPs with the *ID-Sensor*

approach. This is due to the additional information extracted from the low resolution acceleration data in the *ID-Sensor* approach, as shown during an activity transition in Fig. 4, as well as the RSSI pattern associations with the activated ID during static postures such as lying and posture transitions.

Upon close inspection of the instances where false bed-exit events or missed bed-exit events are reported, we identified that they are predominantly due to inadequate tag readings while lying in bed and during getting out of bed. The missed tag readings are a consequence of the *ID-Sensor* being attached to a single shoulder of a patient's loosely fitted garment and not being adequately exposed to the antennas. This can occur as the patient is lying on their side on the bed with the shoulder

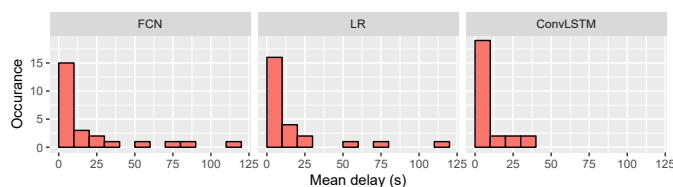


Fig. 7. Bed-exit event recognition delays for the *ID-Sensor* approach

on the mattress. The lack of data or the sparseness in data consequently led to false or missed bed-exit events.

In addition to predicting bed-exits correctly, the system should ideally report bed-exits in a timely manner—with low latency. Figure 7 illustrates the distribution of delays with respect to correctly identified bed-exit events (i.e. TPs). According to the distribution of delays we observed that, for all approaches, the majority of the bed-exit events (> 60%) are identified within a period of 10s with respect to an actual event. However, a classifier that makes a large number of false predictions will likely result in less delays due to constant alarm predictions. This can be seen with the results of ConvLSTM approach where nearly 90% of alarms are with in 10 s. However, we can see from Table II that the ConvLSTM for the *ID-Sensor* approach has high recall but lower precision values indicative of a larger number of false alarms (i.e. FPs).

VII. RELATED WORK

Based on the sensor deployment strategy, we categorize the existing bed-exit recognition systems broadly into: i) environmental sensor-based approaches or device-free methods; and ii) body-worn sensor-based approaches. Given the clinical context of our study, we focus mainly on approaches relevant for detecting bed egress motions as opposed to general activity recognition or human motion detection.

A. Environmental sensors

Studies have investigated the performance of bed-exit alarming systems based on one or multiple sensors strategically placed on or around the bed [9], [11], [33], [34]. Most of these methods involved pressure sensors or pressure mats. In general, pressure mats need daily maintenance to check correct functionality as they are subject to constant mechanical stress and are highly likely to move from their ideal placement on the bed. Moreover, pressure mats require disinfection because of possible exposure to body fluids, and protocols for controlling infections. Additionally, pressure sensors were shown to be unreliable for patients lighter than 45.4 kg (100 lbs) [11]. In fact, two recent randomised control trials evaluating pressure sensor alarms systems to prevent falls found no significant reduction in falls [6], [35]. Both studies reported high false alarms (incorrectly identified alarms) as a significant reason for the negative results.

In contrast Hilbe et al. [33] used bed rails fitted with pressure sensors for bed-exit recognition. However, bed rails can potentially increase harm where a fall may then occur from

a greater height resulting in more serious injury [36] and are no longer considered best practice.

Bruyneel et al. [9] proposed the use of multiple types of commercially available sensors, placed under the bed. These included three sensors to measure the temperature, two piezzo-electric sensors to measure the body movements and three resistive sensors to measure the presence or absence of the patient. The system was evaluated with young healthy participants. Notably, the temperature sensor resulted in a response delay of up to two minutes while it required more than one hour for the system to reach equilibrium between body and mat temperature.

Additionally, commercially available pressure sensor arrays attached to bed mattresses [10] or RFID tags mounted onto walls [37] have been used to analyse sit-to-stand motions. Information from pressure sensor arrays were viewed as image data to identify different phases of the sit-to-stand transitions. Although the focus of these studies was not bed-exit recognition, a sit-to-stand transition may be considered to represent a bed-exit at times [38]. However, further evaluations are required to measure performance for bed-exit recognition, especially with frail older people. The studies above attached sensors to infrastructure rather than individuals, limiting their detection to a specific activity or physical area whilst not solving the *person distinguishability problem* of device free methods [25].

B. Body-worn Sensors

Research studies have looked at kinematic sensors [13], [14], [18], [30], [38], [39] for ambulatory monitoring because of the added possibility of monitoring a person in multiple locations. Most of these studies follow the pioneering study in [14] where a kinematic sensor, composed of one miniature piezoelectric gyroscope and two miniature accelerometers, was attached to a person's sternum to monitor activities such as walking and sit-to-stand posture transitions. However, there is limited research work focused on movement sensor alarm systems for bed-exit recognition [8], [13], [18]. Researchers in [13] used a battery powered acceleration sensor that was strapped with a bandage to the thigh to acquire motion information to identify bed-exit events. The clinical trial in [8] proposed the use of a wearable Bluetooth sensor inserted into a patient vest for determining bed and chair egress movements to realize an alerting system.

Even though battery powered body worn devices generally provide rich sensor data, they are expensive, bulky, obtrusive and require maintenance such as changing or replacing batteries [8]. Further, evidence in the literature highlights the preference for small, unobtrusive and easy to operate monitoring devices by older people [40].

Recently, wearable and batteryless Computational RFID (CRFID) tags capable of supporting embedded sensors have been used to recognize bed and chair egress movements [18], [38]. These studies mainly rely on a MEMS 3D accelerometer sensor data to recognize bed and chair egress movements. Although we have seen the commercialization of CRFID

TABLE IV
PERFORMANCE OF PREVIOUS BED-EXIT MOVEMENT ALARM METHODS

Bed-exit recognition approach	Precision	Recall	Participants' age (years)
Hilbe et al. [33]		96%	18-60
Bruyneel et al. [9]	100%	91%	37±9 and 45±11
Najafi et al. [41]*		93%	66±14
Godfrey et al. [39]*		83%	77.2±4.3
Torres et al. [18]	66.83%	81.44%	71 to 93
Ours	86%	86%	84.4 ±5.3

* a sit-to-stand posture transition was considered as a bed-egress.

technology recently, a wearable CRFID is still undergoing research and development. Further, the per-unit cost of CRFID devices are still several tens of USD. Moreover, these studies show that wirelessly powering a MEMS 3D accelerometer remains a challenging task and leads to loss of information and highly sparse data streams that affect performance of activity recognition algorithms [18].

VIII. DISCUSSION AND CONCLUSION

We have designed a sensing approach using mature COTS UHF RFID technology without the need for a high resolution kinematic sensor employed in previous studies. Our approach provides significant advantages when compared to CRFID devices, battery powered body worn sensors and pressure sensors. COTS passive RFID tags are: *i*) small in size, thus increasing the possibility for integrating the tags into hospital gowns; *ii*) low in cost—0.07 to 0.15 USD [15] and batteryless, thus providing greater economic advantages and increasing the possibility to dispose the tags to support hygiene protocols in hospitals; and *iii*) able to solve the problem of distinguishing individuals and monitoring individuals in multiple locations.

We investigated the efficacy of our *ID-Sensor* approach for recognizing hospitalized fail older people's motions to alert on bed-exits. We have developed a fully convolutional neural network architecture capable of learning information from RFID data streams as opposed to previous applications in wearable sensor data from kinematic sensors. The *ID-Sensor* approach with the FCN dense labelling and prediction approach depicted the highest performance (F-score of 86%). Further, our data was collected in either single- or double-bed rooms, thus suggesting that the approach is *agnostic to the environment across similar antenna deployments*.

Comparisons: In the recent past, several bed-exit systems have been developed. Table IV summarizes the results of previous bed-egress movement recognition approaches, together with our study results. We have excluded pressure mats given the lack of clinical evidence for their efficacy. It is difficult to make a fair comparison with these due to: *i*) differences in the experimental setting such as the characteristics of the study participants and the duration of the study; and *ii*) differences in the performance evaluation measures used. Nevertheless, we can see that the *ID-Sensor* performs comparably better than methods tested with older people.

Studies [9], [33] considered bed exits and reported recall values of over 90%. However, performance reported was based on experiments with young and middle-aged adults while

absence of precision results means that we are unable to comment on false alarms as a function of all alarms. Notably, the empirical methods used were developed and tested with the same dataset; consequently, yielding optimal heuristic measures for the particular dataset. In contrast to a low-cost batteryless RFID tag that can be disposed if required and does not require maintenance re-charging batteries, the sensor required disinfection or thorough cleaning because of possible exposure to body fluids or infection control.

Our results are higher in comparison to studies with body worn batteryless CRFID devices with a high quality 3D accelerometer sensor evaluated with hospitalized older people [18]. Whilst the high resolution accelerometer provided more information, the RF powering issues from various postures from older people and movement such as rolling out of bed by patients resulted in highly sparse data streams. As a consequence, the results show a relatively larger number of false positives compared to our study (66.85% vs. ours 86%).

Limitations: Although our results are promising, our study is not without limitations. During the pilot study, experiments were conducted for few hours using broadly scripted activity routines. Therefore, it is important to validate the results using longer duration trials (such as days opposed to hours), at night as well as daytime. Additionally, we have not evaluated the mean time before failure of the mechanical switch in the *ID-Sensor*.

While the *ID-Sensor* is low cost and has the potential for disposability and textile integration, deploying RFID reader and antenna infrastructure across a hospital is costly and was not discussed here. However, RFID infrastructure (which consists of RFID antennas and readers) is increasingly being deployed in hospitals for patient and asset tracking [42]. Hence, such existing infrastructure is envisioned to be also utilized for patient activity monitoring using an *ID-Sensor*.

Future Work: We leave for future work: *i*) performance evaluation with a sensor integrated hospital gown; and *ii*) the use of two *ID-Sensor* tags over both right and left shoulders of a patient. As a result of the additional information, we expect the tag reading rate to improve and consequently the number of missed tag readings to reduce further to yield higher bed-exit event recognition performance. Further, to establish efficacy, it is necessary to evaluate our approach using a larger study such as a randomised controlled trial.

ACKNOWLEDGMENTS

Our study was supported by a grant from the Hospital Research Foundation and the Australian Research Council (DP160103039). We would like to thank Dr. S. Nair and Mr. S. Hoskin for supporting the trial at the Queen Elizabeth Hospital, South Australia. We would like to acknowledge Mr. R.L. Shinmoto-Torres for collecting and labelling the dataset.

REFERENCES

- [1] World Health Organization. (2017) The global strategy and action plan on ageing and health.

- [2] W. H. Organisation. Falls prevention in older age. [Online]. Available: http://www.who.int/ageing/projects/falls_prevention_older_age/en/
- [3] K. Rapp, C. Becker, I. Cameron, H. Knig, and G. Bchele, "Epidemiology of falls in residential aged care: analysis of more than 70,000 falls from residents of Bavarian nursing homes," *J. A.M. Med. Dir. Assoc.*, vol. 13, no. 2, pp. 187–187, 2012.
- [4] S. N. Robinovitch, F. Feldman, Y. Yang, R. Schonnop, P. M. Leung, T. Sarraf, J. Sims-Gould, and M. Loughin, "Video capture of the circumstances of falls in elderly people residing in long-term care: an observational study," *Lancet*, vol. 381, no. 9860, pp. 47–54, 2013.
- [5] C. S. Florence, G. Bergen, A. Atherly, E. Burns, J. Stevens, and C. Drake, "Medical costs of fatal and nonfatal falls in older adults," *J. of the American Geriat. Society*, vol. 66, no. 4, pp. 693–698, 2018.
- [6] O. Sahota, A. Drummond, D. Kendrick, M. J. Grainge, C. Vass, T. Sach, J. Gladman, and M. Avis, "Refine (reducing falls in in-patient elderly) using bed and bedside chair pressure sensors linked to radio-pagers in acute hospital care: a randomised controlled trial," *Age and ageing*, vol. 43, no. 2, pp. 247–253, 2013.
- [7] R. I. Shorr, A. M. Chandler, L. C. Mion, T. M. Waters, M. Liu, M. J. Daniels, L. A. Kessler, and S. T. Miller, "Effects of an intervention to increase bed alarm use to prevent falls in hospitalized patients: a cluster randomized trial," *Annals of internal medicine*, vol. 157, no. 10, pp. 692–699, 2012.
- [8] R. Visvanathan, D. C. Ranasinghe, A. Wilson, K. Lange, J. Dollard, E. Boyle, J. Karnon, E. Raygan, S. Maher, K. Ingram *et al.*, "Effectiveness of an ambient intelligent geriatric management system (ambigem) to prevent falls in older people in hospitals: protocol for the ambigem stepped wedge pragmatic trial," *Injury prevention*, 2017, online first.
- [9] M. Bruyneel, W. Libert, and V. Ninane, "Detection of bed-exit events using a new wireless bed monitoring assistance," *Int. J. Med. Inform.*, vol. 80, no. 2, pp. 127–132, 2011.
- [10] A. Arcelus, I. Veledar, R. Goubran, F. Knoefel, H. Sveistrup, and M. Bilodeau, "Measurements of sit-to-stand timing and symmetry from bed pressure sensors," *IEEE Trans. Instrum. Meas.*, vol. 60, no. 5, pp. 1732–1740, 2011.
- [11] E. Capezuti, B. L. Brush, S. Lane, H. U. Rabinowitz, and M. Secic, "Bed-exit alarm effectiveness," *Arch. Gerontol. Geriatr.*, vol. 49, no. 1, pp. 27–31, 2009.
- [12] G. Demiris, B. K. Hensel, M. Skubic, and M. Rantz, "Senior residents perceived need of and preferences for smart home sensor technologies," *Int. J. Technol. Assess. Health Care.*, vol. 24, no. 1, pp. 120–124, 2008.
- [13] K.-H. Wolf, K. Hetzer, H. M. z. Schwabedissen, B. Wiese, and M. Marscholke, "Development and pilot study of a bed-exit alarm based on a body-worn accelerometer," *Z. Gerontol. Geriatr.*, vol. 46, no. 8, pp. 727–733, 2013.
- [14] B. Najafi, K. Aminian, A. Paraschiv-Ionescu, F. Loew, C. J. Büla, and P. Robert, "Ambulatory system for human motion analysis using a kinematic sensor: monitoring of daily physical activity in the elderly," *IEEE Trans. Biomed. Eng.*, vol. 50, no. 6, pp. 711–723, 2003.
- [15] RFID Journal, "How much does an RFID tag cost today?" [Online]. Available: <https://www.rfidjournal.com/faq/show?85>
- [16] FUJITSU. Uhf rfid tag wt-a533/wt-a533ht datasheet. [Online]. Available: <http://www.fujitsu.com/us/solutions/business-technology/intelligent-society/rfid/>
- [17] M. Gövercin, Y. Költzsch, M. Meis, S. Wegel, M. Gietzelt, J. Spehr, S. Winkelbach, M. Marscholke, and E. Steinhagen-Thiessen, "Defining the user requirements for wearable and optical fall prediction and fall detection devices for home use," *Inform. Health Soc. Care*, vol. 35, no. 3-4, pp. 177–187, 2010.
- [18] R. L. Shinmoto Torres, R. Visvanathan, D. Abbott, K. D. Hill, and D. C. Ranasinghe, "A battery-less and wireless wearable sensor system for identifying bed and chair exits in a pilot trial in hospitalized older people," *PLOS ONE*, vol. 12, no. 10, pp. 1–25, 10 2017. [Online]. Available: <https://doi.org/10.1371/journal.pone.0185670>
- [19] A. Kiourti, "Rfid antennas for body-area applications: From wearables to implants," *IEEE Ant. and Prop. Magazine*, no. 99, pp. 1–1, 2018.
- [20] B. Jiang, K. P. Fishkin, S. Roy, and M. Philipose, "Unobtrusive long-range detection of passive RFID tag motion," *IEEE Trans. Instrum. Meas.*, vol. 55, no. 1, pp. 187–196, 2006.
- [21] H. Li, C. Ye, and A. P. Sample, "IDSense: A human object interaction detection system based on passive UHF RFID," in *Proceedings of the Human Factors in Computing Systems*, 2015, pp. 2555–2564.
- [22] A. Jayatilaka and D. C. Ranasinghe, "Real-time fluid intake gesture recognition based on batteryless uhf rfid technology," *Pervasive and Mobile Computing*, vol. 34, pp. 146–156, 2017.
- [23] T. Adame, A. Bel, A. Carreras, J. Melià-Seguí, M. Oliver, and R. Pous, "Cuidats: An RFID-WSN hybrid monitoring system for smart health care environments," *Futu. Gene. Comp. Sys.*, vol. 78, pp. 602–615, 2018.
- [24] R. Yao, G. Lin, Q. Shi, and D. C. Ranasinghe, "Efficient dense labelling of human activity sequences from wearables using fully convolutional networks," *Pattern Recognition*, vol. 78, pp. 252–266, 2018.
- [25] C. Wang, J. Liu, Y. Chen, L. Xie, H. B. Liu, and S. Lu, "RF-kinect: A wearable rfid-based approach towards 3d body movement tracking," *Proc. ACM Interact. Mob. Wearable Ubiquitous Technol.*, vol. 2, no. 1, p. 41, 2018.
- [26] H. Jin, Z. Yang, S. Kumar, and J. I. Hong, "Towards wearable everyday body-frame tracking using passive RFIDs," *Proc. ACM Interact. Mob. Wearable Ubiquitous Technol.*, vol. 1, no. 4, p. 145, 2018.
- [27] M. Chesser and D. C. Ranasinghe. (2018) ID-Sensor dataset and code. [Online]. Available: <https://github.com/AdelaideAuto-IDLab/ID-Sensor>
- [28] M. Philipose, J. R. Smith, B. Jiang, A. Mamishev, S. Roy, and K. Sundara-Rajan, "Battery-free wireless identification and sensing," *IEEE Pervasive Comput.*, vol. 4, no. 1, pp. 37–45, 2005.
- [29] P. V. Nikitin, R. Martinez, S. Ramamurthy, H. Leland, G. Spiess, and K. Rao, "Phase based spatial identification of uhf rfid tags," in *International Conference on RFID*, 2010, pp. 102–109.
- [30] L. Wang, T. Gu, H. Xie, X. Tao, J. Lu, and H. Y., "A wearable RFID system for real-time activity recognition using radio patterns," in *Mobile and Ubiquitous Systems: Computing, Networking, and Services*, 2013.
- [31] F. J. Ordez and D. Roggen, "Deep convolutional and lstm recurrent neural networks for multimodal wearable activity recognition," *Sensors*, vol. 16, no. 1, 2016.
- [32] L. Pigou, A. van den Oord, S. Dieleman, M. Van Herreweghe, and J. Dambre, "Beyond temporal pooling: Recurrence and temporal convolutions for gesture recognition in video," *International Journal of Computer Vision*, vol. 126, no. 2, pp. 430–439, 2018.
- [33] J. Hilbe, E. Schulc, B. Linder, and C. Them, "Development and alarm threshold evaluation of a side rail integrated sensor technology for the prevention of falls," *Int. J. Med. Inform.*, vol. 79, no. 3, pp. 173–180, 2010.
- [34] C. D. Vass, O. Sahota, A. Drummond, D. Kendrick, J. Gladman, T. Sach, M. Avis, and M. Grainge, "REFINE (reducing falls in in-patient elderly) - a randomised controlled trial," *Trials*, vol. 10, no. 1, p. 83, 2009.
- [35] R. I. Shorr, A. M. Chandler, L. C. Mion, T. M. Waters, M. Liu, M. J. Daniels, L. A. Kessler, and S. T. Miller, "Effects of an intervention to increase bed alarm use to prevent falls in hospitalized patients: a cluster randomized trial," *Ann. Intern. Med.*, vol. 157, no. 10, pp. 692–699, 2012.
- [36] F. Healey and D. Oliver, "Bedrails, falls and injury: evidence or opinion? a review of their use and effects," *Nursing Times*, vol. 105, no. 26, pp. 20–24, 2009.
- [37] L. Yao, Q. Z. Sheng, X. Li, T. Gu, M. Tan, X. Wang, S. Wang, and W. Ruan, "Compressive representation for device-free activity recognition with passive rfid signal strength," *IEEE Transactions on Mobile Computing*, vol. 17, no. 2, pp. 293–306, 2018.
- [38] A. Wickramasinghe, D. C. Ranasinghe, C. Fumeaux, K. D. Hill, and R. Visvanathan, "Sequence learning with passive rfid sensors for real-time bed-egress recognition in older people," *IEEE Journal of Biomedical and Health Informatics*, vol. 21, no. 4, pp. 917–929, 2017.
- [39] A. Godfrey, A. Bourke, G. laighin, P. van de Ven, and J. Nelson, "Activity classification using a single chest mounted tri-axial accelerometer," *Med. Eng. Phys.*, vol. 33, no. 9, pp. 1127–1135, 2011.
- [40] R. Steele, A. Lo, C. Secombe, and Y. K. Wong, "Elderly persons perception and acceptance of using wireless sensor networks to assist healthcare," *Int. J. of Med. Inform.*, vol. 78, no. 12, pp. 788–801, 2009.
- [41] B. Najafi, K. Aminian, A. Paraschiv-Ionescu, F. Loew, C. Bula, and P. Robert, "Ambulatory system for human motion analysis using a kinematic sensor: Monitoring of daily physical activity in the elderly," *IEEE Trans. Biomed. Eng.*, vol. 50, no. 6, pp. 711–723, 2003.
- [42] A. Prater, M. Bowen, E. Pavich, C. M. Hawkins, N. Safdar, J. Fountain, A. Anderson, M. Frankel, and S. Dehkharghani, "Enhancing workflow analysis in acute stroke patients using radiofrequency identification and infrared-based real-time location systems," *Journal of the American College of Radiology*, vol. 14, no. 2, pp. 231–234, 2017.